



IB/2005/058056

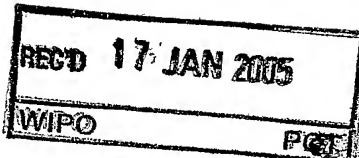

PA 1257058

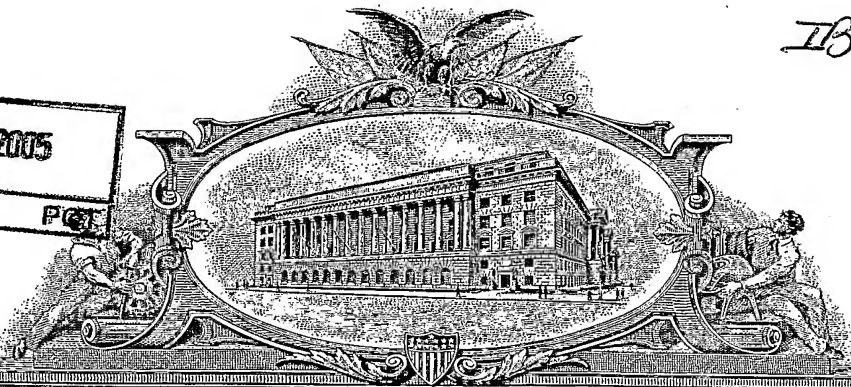

# THE UNITED STATES OF AMERICA

**TO ALL TO WHOM THESE PRESENTS SHALL COME:**

**UNITED STATES DEPARTMENT OF COMMERCE**

**United States Patent and Trademark Office**

**December 09, 2004**


**THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A FILING DATE UNDER 35 USC 111.**

**APPLICATION NUMBER: 60/536,763 ✓**

**FILING DATE: January 15, 2004 ✓**

## **PRIORITY DOCUMENT**

SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH RULE 17.1(a) OR (b)

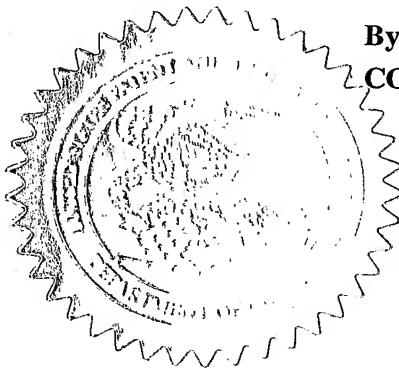

**By Authority of the  
COMMISSIONER OF PATENTS AND TRADEMARKS**

*L. Edelen*

**L. EDELEN  
Certifying Officer**

Approved for use through 10/31/2002. OMB 0651-0032  
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE  
Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

**PROVISIONAL APPLICATION FOR PATENT COVER SHEET**

This is a request for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53(c).

Express Mail Label Number EK419165559US

INVENTOR(S)					
Given Name (first and middle [if any])		Family Name or Surname		Residence (City and either State or Foreign Country)	
James Knox Thomas Dean		Russell Lyster		Bainbridge Island, WA Bothell, WA	
<input type="checkbox"/> Additional inventors are being named on the _____ separately numbered sheets attached hereto					
TITLE OF THE INVENTION (500 characters max)					
Adaptive Physiological Monitoring System and Methods of Using Same					
Direct all correspondence to: CORRESPONDENCE ADDRESS					
<input type="checkbox"/> Customer Number		<input type="text"/>		<input type="text"/>	
OR		Type Customer Number here		Place Customer Number Bar Code Label here	
<input checked="" type="checkbox"/> Firm or Individual Name		Philips Intellectual Property & Standards			
Address		595 Miner Road			
Address					
City		Cleveland	State	Ohio	ZIP 44143
Country		US	Telephone	440-483-4281	Fax 440-483-4874
ENCLOSED APPLICATION PARTS (check all that apply)					
<input checked="" type="checkbox"/> Specification Number of Pages		26		<input type="checkbox"/> CD(s), Number <input type="text"/>	
<input checked="" type="checkbox"/> Drawing(s) Number of Sheets		4		<input type="checkbox"/> Other (specify) <input type="text"/>	
<input type="checkbox"/> Application Data Sheet. See 37 CFR 1.76					
METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT					
<input type="checkbox"/> Applicant claims small entity status. See 37 CFR 1.27.				FILING FEE AMOUNT (\$)	
<input type="checkbox"/> A check or money order is enclosed to cover the filing fees					
<input checked="" type="checkbox"/> The Commissioner is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number:		14-1270		\$160.00	
<input type="checkbox"/> Payment by credit card. Form PTO-2038 is attached.					
The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.					
<input checked="" type="checkbox"/> No.					
<input type="checkbox"/> Yes, the name of the U.S. Government agency and the Government contract number are: _____					

Respectfully submitted

SIGNATURE



TYPED or PRINTED NAME Thomas M. Lundin, Esq.

TELEPHONE 440-483-4281

Date 01/15/2004

REGISTRATION NO.  
(if appropriate)  
Docket Number:

48,979

PHUS040020USP

**USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT**

This collection of information is required by 37 CFR 1.51. The information is used by the public to file (and by the PTO to process) a provisional application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the complete provisional application to the PTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, Washington, D.C. 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Box Provisional Application, Assistant Commissioner for Patents, Washington, D.C. 20231.

**UNITED  
STATES  
PROVISIONAL  
PATENT  
APPLICATION**

**ADAPTIVE PHYSIOLOGICAL  
MONITORING SYSTEM AND  
METHODS OF USING SAME**

**INVENTORS:**

James. K. Russell and Thomas D. Lyster

**ADAPTIVE PHYSIOLOGICAL MONITORING SYSTEM AND  
METHODS OF USING THE SAME**

5     **FIELD OF THE INVENTION**

        The present invention relates generally to the field of physiological monitoring of patients, and more particularly, to methods and an apparatus for a physiological monitoring system with an adaptive alert mechanism.

10    **BACKGROUND**

        Doctors often need round-the-clock measurements of a body parameter over a period of time to make an accurate diagnosis of a condition. Vasovagal syncopal events and arrhythmias of the heart are particularly challenging to diagnose because of their relative infrequency, sudden onset and short duration. Holter monitors are one type of  
15    ambulatory physiological monitoring systems (PMS) that are used to measure the electrical signals of a patient's heart over a period of time to detect abnormalities in the heart beat of the patient. Typically, these systems continuously monitor electrocardiography (ECG) signals for a finite test period of about 24-96 hours. By reviewing the collected ECG data in an external monitoring device, doctors may identify patients who have heart arrhythmias  
20    and who are at risk for ventricular tachycardia or other cardiac conditions.

        In patients who have already been diagnosed with an arrhythmic heart condition, and who are at risk for potentially life-threatening cardiac events, it is often desired to monitor their condition over the long term. It is therefore desirable that the monitoring system be capable of long term monitoring for arrhythmic events and adequately capture  
25    such events when they occur. Since the device will be worn by the patient for potentially

5 long durations of time, it is also desirable for the device to be compact, lightweight, mechanically robust, and unobtrusive as the patient goes about his normal daily routine of activity and rest. Traditional Holter monitors are unsuitable for such long term monitoring because of their bulky profile and relatively high power consumption levels required to power the continual ECG detection and data storage.

10 Ambulatory ECG monitors typically include several electrodes that are attached to the patient and a processor that acquires and processes the electrical signals into data and stores the data for later analysis. If it is functioning properly, the monitoring system is able to detect and capture cardiac event data for later retrieval and analysis. In practice, however, it is often the case that the monitoring becomes interrupted because of battery-  
15 power loss, sensor detachment problems, or other system or user errors.

Existing PMS typically employ an audible or visual alarm to alert the user of any such system malfunctions or errors. Some of the malfunctions or errors that trigger the alarm require immediate user attention, such as a malfunction requiring shutdown and restart of the PMS, signal loss due to improper sensor connection(s), or electrical  
20 interference. Other errors that trigger the alarm are less urgent (e.g., low battery power). In these prior art systems, both urgent and non-urgent types of information are communicated to the user via the alarm, whether or not the user is receptive to being disturbed.

One such conventional system is described in U.S. Patent No. 6,248,067 to Causey, Kovelman, Purvis, and Mastrototaro, and assigned to MiniMed Inc., which patent is  
25 entitled "Analyte Sensor and Holter-Type Monitor System and Method of Using the Same," which is hereby incorporated by reference in its entirety. This patent describes a Holter-type recorder device equipped with a vibrator alarm or optical indicator such as a light-emitting diode (LED) that alerts the user of a system malfunction. This vibration

5 alarm, if it remains unanswered by the user, provides additional reminders to an audio alarm. The drawback of this system is that the audio alarm may become triggered during periods of sleep or other inopportune times when the user cannot respond promptly.

In other systems, a user of the PMS may manually change a switch setting between audible and/or silent (e.g. tactile or visual) alarm modes to prevent undesired beeping  
10 interruptions. However, manual switching represents a suboptimal solution because the burden is on the user to constantly switch between modes as he goes about his daily routine of active and inactive periods and other instances where interruptions may not be tolerated or it is necessary to conceal the presence of the PMS.

There is a need, therefore, for an improved method and apparatus for an adaptive  
15 physiological monitor that alerts the user of events indicating a system problem or malfunction when it determines that the user is in an active waking state or otherwise receptive of receiving and responding to the alarm.

In the case of PMS systems that alarm for life-threatening arrhythmia conditions, physical activity on the part of the monitored patient has some additional implications.  
20 First, physical activity may result in signal artifact that causes the monitored physiological parameter (e.g. the ECG signal) to resemble its form when some life-threatening arrhythmias (e.g. ventricular fibrillation) are present when they are in fact absent, and may generate a false positive alarm. At the same time, physical activity above a certain level may be inconsistent with the presence of the life-threatening arrhythmia or condition,  
25 because the life-threatening condition weakens the patient or renders the patient unconscious. Thus, physical activity itself, apart from its influence on the signal quality of the monitored physiological parameter, provides significant information about the patient's

5 cardiac status, and in combination with the ECG signals, provides a more complete assessment of the cardiac condition of a patient at a given time.

Accordingly, there is also a need for a knowledge-based PMS that inhibits the transmission of an alarm reflecting a life-threatening physiological event when the system detects that the patient is physically active.

10

#### SUMMARY OF THE INVENTION

The present invention solves these and other problems by providing a method and apparatus for an adaptive physiological monitoring system that differentiates between urgent and non-urgent information and then alerts the user accordingly based on a  
15 knowledge-based approach that considers the user's receptivity to responding to the information, and more generally that considers the implications of the user's level of physical activity. By transmitting information in this adaptive manner, user acceptance of the PMS is improved. The user is not disturbed during periods of rest with non-urgent information, and the incidence of false positive alarms is reduced as well.

20 According to one aspect of the present invention, an exemplary embodiment is a method and system for an adaptive physiological monitoring system that monitors one or more physical parameter(s) of the user to distinguish between periods of quiet rest and normal waking activity and communicates non-urgent information to the user only if one or more physical parameters of the user exceeds a predetermined threshold.

25 According to an embodiment of this aspect of the present invention, the physiological monitoring system incorporates a sensor responsive to the physical activity level of the user, such as an accelerometer or other mechanical, chemical, or electrical means for detecting directly or indirectly measuring the physical activity level of the user

5           According to another aspect of the invention, an exemplary embodiment is a method and apparatus for a lightweight, energy-saving physiological monitoring system that conserves power by delaying transmission of non-urgent information to the patient when the patient is asleep or resting.

          According to one embodiment of this aspect of the present invention, the alert  
10 information is communicated to the patient by means of a device local to the monitor, such as a vibrator or speaker.

          According to another embodiment of this aspect of the present invention, the alert information is communicated to the patient by means of devices in his environment, which the monitor signals wirelessly.

15           According to yet another aspect of the invention, an exemplary embodiment is a method and apparatus for long term, low power ECG monitoring. By limiting the transmission of information when the patient is asleep or resting, the present invention allows for considerable savings in battery power consumption, increasing the capacity for long term monitoring of the patient.

20           According to yet another aspect of the invention, an exemplary embodiment is a method and apparatus for long term monitoring for life-threatening physiological events. By inhibiting the transmission of alarms reflecting the appearance of a life-threatening pattern in the physiological parameter being monitored when the patient is engaged in normal waking activity inconsistent with the life-threatening phenomenon, the incidence of  
25 false alarms is reduced.

#### BRIEF DESCRIPTION OF THE DRAWINGS



5           FIG 1 is a perspective view of one embodiment of the physiological monitoring system of the present invention.

          FIG 2 is a pictorial view showing a physiological monitoring system (PMS) according to an embodiment of the present invention on a patient.

          FIG 3 illustrates a block diagram depicting the major components of the PMS  
10   according to an exemplary embodiment of the present invention.

          FIG 4 is a flow chart depicting the steps performed by the physiological monitoring system to create a feedback loop that monitors a patient's physiological parameters and alerts the patient of system errors and physiological conditions in an adaptive manner based on the detected activity level of the patient.

15

#### DETAILED DESCRIPTION OF PREFERRED EMBODIMENTS

          A more complete understanding of the method and apparatus of the present invention is available by reference to the following detailed description of the embodiments when taken in conjunction with the accompanying drawings. It is worthy to  
20   note that any reference herein to "one embodiment" or "an embodiment" means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment of the invention. The appearances of the phrase "in one embodiment" in various places in the specification are not necessarily all referring to the same embodiment. The detailed description of the embodiments which follows is  
25   intended to illustrate but not limit the invention. The scope of the invention is defined by the appended claims.

          A physiological monitoring system according to the present invention comprises an adaptive system that, in addition to monitoring a particular physical characteristic of the

5 patient for medical purposes, communicates a variety of information to the user based on a knowledge-based approach that determines whether the user is physically active. If the system detects that the patient is asleep, resting, or otherwise in a non-active state, it defers the transmission of non-urgent information until it detects that the patient is in a normal active state. On the other hand, if the system detects that the patient is in a normal active state, it inhibits, as false alarms, transmission of any urgent information that is inconsistent  
10 with the patient being in a normal active state.

Briefly, the above-described adaptive monitoring is achieved by way of an internal microprocessor having sufficient logic and data analysis capabilities to independently perform all internal control functions, including acquisition of data from sensors,  
15 processing of that data, and providing appropriate instructions to various sensors and output devices. On-board memory (e.g., static read and write memory) performs control and analysis processes and selectively stores critical information regarding a cardiac episode.

FIG 1 illustrates a perspective view of an embodiment of the monitoring system for  
20 monitoring cardiac parameters in an ambulatory setting of daily activity. The system 10 comprises a monitor 100 and sensors 110 or other transducers that are connected to the monitor 100. A wireless transmitter 109, and optionally, an event button 104 are located on the monitor 100.

The monitor 100 is designed for use with one or more sensors or transducers such  
25 as electrodes 112. As will be appreciated by one of skill in the art, a variety of sensors may be employed in the practice of this invention. With sufficient hardware and connections to the body, numerous physiologic parameters may be sensed as is pointed out in U.S. Pat. No. 5,464,434 issued to Alt and U.S. Pat. No. 5,464,431, issued to Adams et

5 al., which is hereby incorporated by reference in its entirety. The physical parameters may include, but are not limited to, a patient's body movements, heartbeats, respiratory movements, snoring, and other mechanical movements and sounds detected by the sensors, respiration rate and depth (by for example, impedance plethysmography), brain waves, body temperature, and blood pressure.

10 A plurality of sensors 110 may be employed simultaneously to measure the same or different physiological characteristics. For instance, typically two to six electrodes 112 may be employed to measure biological rhythmic signals such as heart rate in conjunction with an activity sensor 114 such as an accelerometer that measures the physical activity level of the patient. As shown in FIG 2, in one embodiment, at least one set of sensors 110  
15 comprises ECG electrodes 112 that measure electrocardiograms and that are placed in contact with the patient's body so as to receive signals from the patient which are transmitted to the monitor 100. As is obvious to one of skill in the art, the electrodes may be conventional electrodes comprised of silver chloride or other compositions designed to receive analog ECG input. The system 10 may also comprise a set of activity sensors 114  
20 that detect motion, movement, acceleration, mechanical vibrations, sound, or other indicator of physical activity on the part of the human subject.

The activity sensor 114 may comprise a piezoelectric pressure transducer, a pedometer, a vibratory or motion detector, a detector that measures residual noise generated by friction between the electrode contacts and the patient's skin, strain gage or  
25 other transducer means for measuring activity. In addition to an accelerometer, other sensors which measure physiological parameters which distinguish between resting and active states may be employed.

5           In one mode of the invention, the activity sensor 114 is a cantilevered suspended element which constitutes a high impedance voltage generator such as a piezoelectric element. The sensors may be incorporated into the monitor module 100 itself, or placed in close proximity to the monitor. The output of the activity sensor 114 is connected to a processor 142 contained within the monitor 100. The piezoelectric element is a passive  
10   element or sensor requiring no power to cause it to be operational. The distortion of the surface of or of the element, itself, generates the appropriate signal.

          The activity sensors 114 may alternatively detect chemical or electrical changes in the patient that indicate the onset of sleep. For example, in one exemplary embodiment, the activity sensor 114 is integrated within the monitor 100 unit, as shown in FIG 2, and in  
15   other embodiments, are external to the monitor 100, such as a wrist-mounted activity sensor 114 attached to a wrist with a strap that detects electromyographic (EMG) electrical impulses produced by the wearer's wrist muscles. Such electrical impulses provide measurements of the changes in the muscular activity at the wearer's wrist, which measurements are useful in detecting drowsiness. The sensors 110 are applied to the body  
20   such that the surface of the sensors makes physical and/or electrical contact with the patient.

          Although the monitor 100, and thus the sensors 110 are shown applied to the chest, one of skill in the art will appreciate that various alternative sensor construction, materials, and designs are within the scope of the present invention. The information signals from  
25   these measuring devices such as the ECG electrodes 112 and activity sensors 114 are then transmitted to the monitor 100 for amplification and processing.

          Referring now to FIG 3, which is a block diagram of the major elements of the monitoring system 10, the system includes the sensors 110 (sensor electrodes 112 and

5 activity sensor 114), an electronics module 140, a power circuit 150, which provides power to the system 10, and may include a voltage splitter and voltage regulator in addition to a battery, an alarm 160 (acoustic alarm 162 and silent alarm such as a tactile or visual/light alarm 164), a user interface module 170, a wireless transmitter 109 or other means for communicating with an external computer, device, or medical personnel (not shown). The user interface module 170 includes an event button 104 and optionally, a user display 106 which displays status messages and system error messages to the user.

Referring now to the details of the exemplary electronics module 140 shown in block form in FIG 3, the major components of the electronic module 140 include a CPU or microprocessor 142 with an internal CPU memory 144 and an internal digital input/output circuit, signal conditioners 145, analog-to-digital converters 147, an activity threshold detector 148 input with a programmable activity level 149, and a clock 146. The microprocessor 142 performs a multitude of functions, including, but not limited to, receiving and processing signals output from the sensors 110 regarding arrhythmia conditions and checking and processing system errors. The selection and design of such circuitry and various other circuit means will be obvious to one of ordinary skill upon review of this specification.

The output of the sensors 110 such as the ECG electrodes 112 is coupled to a signal conditioning circuit 145 which filters and amplifies the output. For the purposes of this example, the present invention contemplates that the ECG electrode sensors 112 and activity sensor 114 are analog signals that are communicated to an analog-to-digital (A/D) converter and communicated to the microprocessor 40 as digital signals along signal path 141. Digital sensors may be substituted, bypassing the A/D converter 147.

5           Communication between the microprocessor 142 and memory/storage 144 is provided by memory line 143. The data storage (memory) device 144 is optionally included for storing the ECG signal data, pre-set threshold limits for the physiological conditions being monitored, and user input received through the user interface module 170.

10           In the interest of keeping the monitor 100 compact and lightweight, the memory 144 may be limited to internal CPU/microprocessor memory, which for example, may be static random access memory or "flash" memory, their equivalents, or any of the above in combination with conventional magnetic storage such as a small portable disk drive unit. If the memory comprises only an internal CPU flash memory with limited data storage capacity, the ECG signal data detected by electrodes 112 may be stored into memory in a  
15           continuous overwrite mode.

          In the present embodiment, flash memory (e.g., 128K of SRAM) is provided. Under normal circumstances when no arrhythmia event is occurring, the monitoring system 10 continuously overwrites the ECG data in the CPU flash memory. When an arrhythmia event does occur, the monitoring system 10 retains the data for the short time  
20           period surrounding the event (e.g. 1 minute) in the memory for later study. As will be appreciated by one of skill, the information may be stored in reserved areas of a looping memory, preferably in identifiable memory partitions and accessed in sections or in its entirety with the appropriate external device to initiate and receive such transmissions from the monitoring system 10. Event recording using such a looping memory is detailed in the  
25           prior art such as in U.S. Patent No. 5,987,352 to Klein, Warkentin, Riff, Lee, Carney, Turi, and Varrichio, and assigned to Medtronic, Inc., which patent is entitled "Minimally Invasive Implantable Device for Monitoring Physiologic Events," which is hereby incorporated by reference in its entirety.

5           For each physiological parameter that is being monitored by the sensors 110, an individualized baseline or threshold may be computed and stored in the RAM memory of the microprocessor 142 or an optional external memory 144. In the case of some physiological parameters, fixed threshold levels may be used. The microprocessor 142 receives status information from the memory 144 regarding these system variables. In an  
10   exemplary embodiment, information regarding the arrhythmia frequency that is pre-determined to qualify as a class 1 arrhythmia event is stored in the flash memory of the microprocessor 142. If the ECG sensors measure electrical signals that exceed the programmed arrhythmia frequency, the microprocessor 142 alerts the patient through the user interface module 170, and/or with external devices through the wireless transmitter  
15   109. In the case of alerts reflecting states in which the patient may require assistance, or may be unresponsive, alerts may instead or additionally be directed, by means of wireless transmission to an external system, such as to an emergency responder.

          The user interface 170 communicates with the microprocessor 142 of the electronics module 140 via an internal digital input/output circuit which communicates  
20   directly with the microprocessor 142 on input/output lines. For instance, when the battery power is low (e.g., depletion within 24 hours of usage), the microprocessor prompts a message on the user display 106, warning the user that the battery power needs to be recharged. The user display 106 is a visual display that may be implemented as a light-emitting diode (LED) display, a dual-colored (back to back) LED, or a conventional alpha-  
25   numeric display such as a liquid crystal display (LCD). In the single LED embodiment, the microprocessor may cause the LED to flash to indicate low battery power or a system error. In a dual-colored LED embodiment, the microprocessor 142 may cause the LED to remain unlit and flash in two different colors to indicate the status of the battery power or

5 other system functions. If an LCD is employed, the display may indicate the time of day as well as system status information.

In some embodiments, the pressing of the optional event button 104 by the ambulatory patient causes the user interface 170 to send a signal to the microprocessor 142 to trigger the acoustic alarm 162 which emits an audible alarm and optionally transmits an  
10 alarm signal to a wired or wireless transceiver or other external communication device (not shown) for contacting appropriate medical personnel. In addition, actuation of the event button 104 may cause the microprocessor 142 to record the time an event such as the suffering of chest pains or heart flutters occurred so that the ECG data recorded at that time can be flagged for closer examination. Pressing the event button 104 also causes the  
15 microprocessor 142 to store the ECG data sequence of the event in the flash memory of the microprocessor 142 for later transmission to an external monitoring device (not shown) and later study. In the event of a false alarm, the optional event button 104 may also be used to contact and to cancel the emergency help.

The acoustic alarm 162 also emits an acoustic signal when an observed  
20 cardiovascular activity or other physiological parameter surpasses a preset limit (e.g., surpassing the maximum number of arrhythmias preset by the doctor will generate an alarm). In the case of a physiological state that is inconsistent with normal physical activity on the part of the patient, if the activity monitor threshold is exceeded, such an alert may be suppressed as a false alarm.

25 The output of the sensors 110 (electrode sensors 112 and activity sensor 114) is coupled to a signal conditioning circuit 145, which amplifies and filters the signals, and converted to a digital format by the analog/digital converter. The signals from the activity sensor 114, once digitally processed, are input into an activity threshold detector 148,



5 which is coupled to the A/D converter 147. The flow of signals and activity threshold detector 148 are set to a selected activity level by programmable activity level 149. The activity threshold detector 148 is connected to a control circuit in the microprocessor 142. The output of activity threshold detector 148 may be in binary form. For example, it may be a binary 1 if a threshold level of activity is sensed and a binary 0 if less than the  
10 threshold level of activity is sensed. The binary signal is fed to the control circuit of the microprocessor 142, which operates to power the alarm system 160. Multiple activity thresholds may be employed, establishing separate control levels for the separate adaptive functions of controlling non-urgent communication and urgent communication.

FIG 4 illustrates a flow chart of a method performed by the system 10 during  
15 adaptive monitoring of the patient according to an embodiment of the present invention. The microprocessor 142 initially sets up system variables in its memory so that the variables are proper for operation (step 200). For instance, data relating to the threshold conditions for each physiological parameter are entered into the memory of the microprocessor 142 serving the monitor 100. Thus, pre-determined baseline information  
20 regarding arrhythmia, such as the frequency and signal amplitude of electrocardiograms that would constitute a class 1 arrhythmic event are stored in the flash memory of the microprocessor 142. It is also within the scope of this invention to utilize algorithmic routines to calibrate non-static, non-preset thresholds that adapt to changing physical parameter base line information.

25 The system is also set so that various types of system errors, malfunctions or low power level (hereinafter collectively referred to as "errors") are categorized as either urgent or non-urgent and this information is contained in the memory. In an exemplary embodiment of the physiological monitoring system 10 of the present invention, the

5 microprocessor 142 runs an error routine to check for errors. Based on pre-set information, it recognizes whether an error that has occurred is "urgent" (e.g., hardware or software malfunction, system crash, corrupted data, or other error that requires the user to reinitialize the system or to obtain technical servicing of the module) or "non-urgent" (e.g., signal loss from one of the several electrode sensors due to detachment from the patient's  
10 body, warning that 24 hours of battery operating time remains, or static or electrical interference issues) that will need eventual, but not immediate patient attention.

When the monitor 100 is powered up, the microprocessor 142 executes an initialization routine to prepare the monitor unit for operation (step 210). Part of the initialization routine is for the microprocessor 142 to perform power up tests of the monitor  
15 100 and controls of the user interface 170, including the event button 104 and user display 106. If the system fails any of the power up tests, the microprocessor 142 idles and prompts status messages on the visual display through the user interface 170.

If the system checks were successfully completed, the system enables a data acquisition mode (step 220). During the data acquisition mode, the system 10 receives and  
20 processes information from the electrode sensors 112 and continuously overwrites the ECG data in the CPU flash memory 144. Although it is within the scope of this invention to do so, to conserve memory and processing power, the activity data from the activity sensors 114 is not recorded. The data acquisition mode also includes receiving and processing information about the activity level of the patient output from the activity  
25 sensor 114. As described above, the output from the activity sensor 114 is processed through an activity threshold detector.

The monitoring continues until signals from the electrode sensors exceed a pre-set threshold, and thus indicate a "cardiac event," (step 230). The microprocessor 142

5 determines whether the signals indicate a cardiac event of the type that is life-threatening regardless of the physical activity level of the patient, or of another type that is life-threatening only if physical activity level is below a pre-set threshold. For cardiac events that are inconsistent with normal physical activity on the part of the patient (e.g., cardiac event is of the type that should not trigger an alarm condition if it is detected while the  
10 patient is physically active), the microprocessor 142 processes the output of the activity threshold detector 148.

If the microprocessor 142 determines that the measured signal level is above a pre-programmed activity threshold for a predetermined period of time (which may be medically and experimentally determined), indicating that the patient is in an alert state,  
15 the microprocessor 142 may suppress the cardiac event alert and return the system to the monitoring state 220. However, if in addition to exceeding the pre-set threshold for the electrode sensors, the activity level is below the set variable threshold (step 240), indicating that the patient is inactive, and has probably been rendered unconscious by the cardiac event, the microprocessor 142 does not suppress the cardiac event alert.

20 In certain embodiments of the invention, the PMS may be programmed with additional pre-set thresholds that recognize a variety of ECG signals and patterns that indicate a cardiac event even when physical activity is detected on the part of the patient. In such instances, when ECG signals of a pre-determined type exceed the pre-set threshold, the cardiac event alerting will remain unsuppressed regardless of the patient's activity  
25 level.

When an unsuppressed cardiac event occurs, the microprocessor 142 records the time from clock 146, turns off the ECG data overwriting routine and saves ECG data relating to the cardiac event and a buffer time period before and after the event (e.g., 30

5 seconds before and 30 seconds after the event) in the flash memory of the microprocessor 142 for later transmission to an external monitoring device (not shown) and later study (step 250). It also signals the alarm circuit 160 to trigger the acoustic alarm 162 and sends a distress signal through the wireless transmitter 109 (step 260). The acoustic alarm continues to sound an alarm signal until it turned off by the patient or the doctor (step 270).

10 If neither of the above events has occurred after a pre-set time interval of monitoring has occurred, the microprocessor 142 processes error routines (step 290).

At step 290, the microprocessor 142 checks for system errors and malfunctions and conducts a test for the battery power level. If any type of system error is detected during the error routine, the microprocessor 142 determines, based on the information in the

15 memory 144, whether the error is urgent or non-urgent (step 300). If it is urgent, the microprocessor 142 sends a signal to trigger the acoustic alarm 162 and wireless transmitter 109 (step 310). However, if a non-urgent error is detected, the microprocessor 142 processes the output of the activity threshold detector 148.

If the microprocessor 142 determines that the measured signal level is above a pre-

20 programmed activity threshold for a predetermined period of time (which may be medically and experimentally determined), indicating that the patient is in an alert state, the microprocessor 142 may sound an acoustic alarm 162 and wireless transmitter 109 to alert the patient to system malfunctions or errors requiring immediate attention. However, if the activity level drops below the set variable threshold (step 320), indicating that the

25 patient is asleep or resting, the microprocessor 142 triggers a silent alarm such as a visual message on the user display 106 (step 330). The system 10 is designed to continue to monitor the patient normally until the activity level rises above the activity threshold, in which case, the system triggers the acoustic alarm (step 260).

5           Although various embodiments are specifically illustrated and described herein, it  
will be appreciated that modifications and variations of the invention are covered by the  
above teachings and are within the purview of the appended claims without departing from  
the spirit and intended scope of the invention. For example, specific electrodes for the  
monitoring system are depicted herein, yet other sensors are possible without departing  
10   from the scope of the present invention. Substitute sensors that detect physiological  
characteristics that function similarly to electrodes will be obvious to one of ordinary skill  
in the art. Moreover, while three electrodes are shown, other numbers of electrodes can be  
used without departing from the scope of the present invention. Furthermore, these  
examples should not be interpreted to limit the modifications and variations of the  
15   invention covered by the claims but are merely illustrative of possible variations.

CLAIMS:

1. A physiological monitoring system (10) which comprises:
  - at least one sensor for detecting a biological signal (112), representative of a physiological characteristic of a monitor-wearing patient and generating an electrical signal representative of the biological signal;
  - at least one sensor for detecting the physical activity of the patient (114) and generating an electrical signal, representative of physical activity;
  - processing means (142), coupled to said sensors (112, 114) for processing said electrical signals;
  - an activity threshold detector (148) coupled to said processing means (142) for receiving said electrical signals representative of physical activity;
  - means for testing system functions;
  - a user interface (170) for communicating information about the detected biological signal and system functions to the patient;
  - means for controlling the communication of information (109) in response to detection of an activity threshold by said activity threshold detector (148).
2. The system of claim 1, further comprising a means for programming said physical activity sensor 114 for operational control at a selected threshold of physical activity.
3. The system of claim 1, wherein the physiological characteristic sensor (112) is adapted to sense cardiac signals.

4. The system of claim 1, wherein the physiological characteristic sensor (112) comprises electrocardiography electrodes that detect biological signals representative of the heart beats of the patient.

5. The system of claim 1, wherein the physical activity sensor (114) comprises a transducer that detects chemical, electrical or mechanical characteristics of a monitor-wearing patient, representative of physical activity, including vibrations, motion, acceleration, electromyographic impulses, or sound impulses.

6. The system of claim 1, wherein the physical activity sensor (114) comprises an accelerometer, a pedometer, an electrical noise detector, electronic capacitive sensor, an electromyographic sensor, a skin impedance sensor, or a piezoelectric sensor.

7. The system of claim 1, wherein the physical activity sensor (114) is a passive transducer including a piezoelectric element.

8. The system of claim 1, further comprising a means for wireless transmission of information (109) about the detected biological signal or system functions to a receiver external to the system.

9. An ambulatory electrocardiography monitoring system (10) for recording electrocardiography signals from a patient, comprising:

a plurality of sensors (110) for detecting a plurality of biological signals, each biological signal representative of a physiological characteristic of a monitor-wearing

patient, wherein at least one sensor (110) comprises a one or more electrocardiography electrodes (112) that sense electrocardiography signals from a patient and at least one sensor (110) comprises a sensor that detects the activity level of the patient (114), whereby the sensors generate an electrical signal representative of each respective biological signal;

an arrhythmia threshold detector (142) coupled to the electrocardiography sensor (112) for receiving said electrical signals representative of the electrocardiography signals and determining whether the signals are below or above a preset threshold;

an activity threshold detector (148) coupled to the activity sensor (114) for receiving said electrical signals representative of the activity level of the patient and determining whether the signals are below or above a predetermined threshold;

system error detector (142) for detecting system errors, including signal loss, electrode detachment from patient, low battery power, corrupted data, or electrical interference and determining if the detected error meets pre-determined criteria;

processor (142) for controlling the communication of system and biological signal information to the patient through a user interface (170) based on the detection of an activity threshold by said activity threshold detector (148), arrhythmia threshold by said arrhythmia threshold detector (142), and/or system errors by the system error detector (142).

10. The system of claim 9, wherein the user interface (170) comprises an alarm circuit (160) comprising acoustic, tactile, or visual modes of communicating information to the patient, and mode is determined by processor (142) based on whether the signals from the respective detectors (142, 148) meet pre-determined thresholds.



11. The system of claim 9, wherein processor (142) further comprises a calibration means for setting the threshold of the arrhythmia threshold detector (142) based on processing of electrocardiography signals from the patient to generate a baseline of electrocardiography information.

12. The system of claim 9, wherein the threshold of the arrhythmia threshold detector (142) is pre-programmed into a memory component (142, 144) of the system (10).

13. The system of claim 9, wherein the physical activity sensor (114) comprises a transducer that detects chemical, electrical or mechanical characteristics of a monitor-wearing patient, representative of physical activity, including vibrations, motion, acceleration, electromyographic impulses, or sound impulses.

14. The system of claim 9, wherein the physical activity sensor (114) comprises an accelerometer, a pedometer, an electrical noise detector, electronic capacitive sensor, an electromyographic sensor, a skin impedance sensor, or a piezoelectric sensor.

15. The system of claim 9, wherein the physical activity sensor (114) is a passive transducer including a piezoelectric element.

16. The system of claim 9, wherein the arrhythmia threshold detector (142) is set at a pre-determined threshold to detect the occurrence of class 1 arrhythmia event.

17. The system of claim 9, further comprising means of wireless communication (109) to an external system, for communication of information about the patient and system state to the patient or to others.

18. A method for communicating information about a patient during ambulatory monitoring of a physiological condition of the patient comprising the steps of:

- attaching a physiological monitoring system (10) to a patient;
- sensing one or more selected physiological parameters of the patient;
- sensing the physical activity of the patient;
- comparing the sensed physical activity to a pre-set threshold to determine whether the physical activity exceeds the threshold;
- detecting a system error to be communicated to the patient and determining whether the detected error meets pre-determined criteria;
- generating an error signal based on the system error and transmitting the error signal to the patient via a user interface (170), if the physical activity of the patient exceeds the pre-set threshold.

19. The method of claim 18, wherein the physical activity sensor (114) comprises a transducer that detects pre-determined chemical, electrical or mechanical characteristics of a monitor-wearing patient that are representative of physical activity, wherein the characteristics comprise vibrations, motion, acceleration, electromyographic impulses, or sound impulses.

20. The method of claim 18, wherein the physical activity sensor (114) comprises an accelerometer, a pedometer, a noise detector, electronic capacitive sensor, an electromyographic sensor, or a piezoelectric sensor.

21. The method of claim 18, wherein the selected physiological parameter of the patient is sensed by at least one sensor (110) comprising two or more electrocardiography electrodes (112) that sense electrocardiography signals from the patient, whereby the sensor (110) generates an electrical signal representative of the selected physiological parameter.

22. The method of claim 18, wherein the physiological parameter comprises electrocardiography signals and the threshold of the selected physiological parameter of the patient is detected by an arrhythmia threshold detector (142) that determines whether the sensed electrocardiography signals are below or above a selected threshold representing an arrhythmic event.

23. A method for communicating information about a patient during ambulatory monitoring of a physiological condition of the patient comprising the steps of:

- attaching a physiological monitoring system to a patient;
- detecting a selected physiological parameter of the patient
- sensing the physical activity of the patient;
- detecting a selected threshold of the physical activity of the patient;
- comparing the detected physiological parameter with pre-determined criteria to determine a physiological state of the patient reflecting an alarm condition;


PHUS040020USP


generating an alert signal if the physiological condition of the patient reflects an alarm condition; and

transmitting the signal to the patient via a user interface (170), if the physical activity of the patient is below the selected threshold.

ABSTRACT

The present invention provides methods and an apparatus for an adaptive physiological monitoring system (10). The physiological monitoring system incorporates a sensor (110) responsive to the physical activity of the monitor-wearing patient. The system monitors one or more physical parameter(s) of the user to distinguish between periods of quiet rest and normal waking activity and communicates non-urgent information regarding a system error or information about the measured physical parameter to the user or to an external system only if one or more physical parameters of the user exceed predetermined threshold criteria. The system also suppresses alerts regarding physiological states that are inconsistent with normal patient activity if one or more physical parameters of the user exceed a predetermined threshold. The physiological monitoring system (10) incorporates a sensor (110) responsive to the physical activity level of the user, for detecting directly or indirectly measuring the physical activity level of the user.

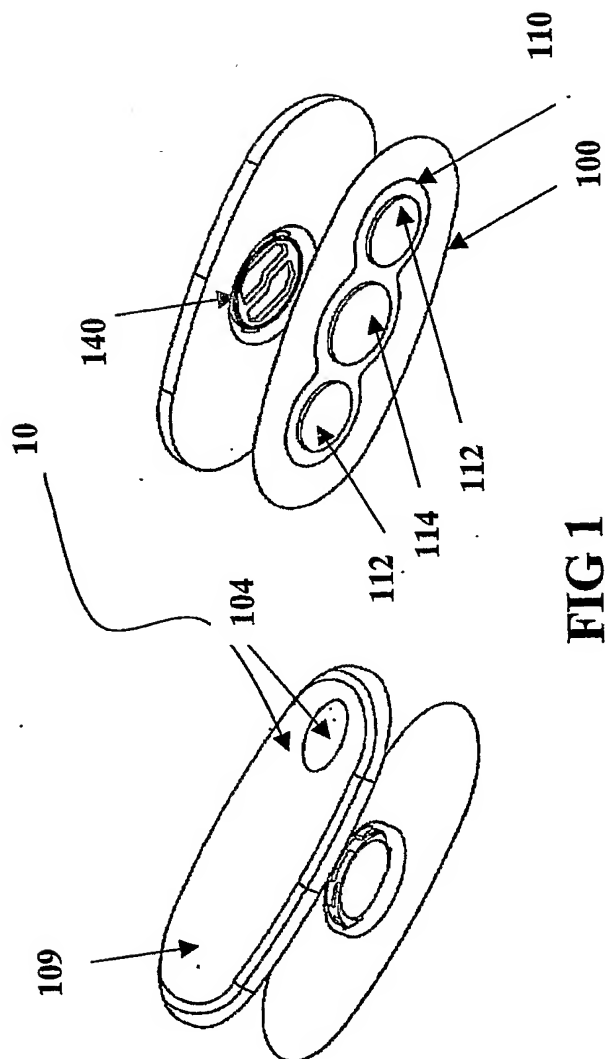

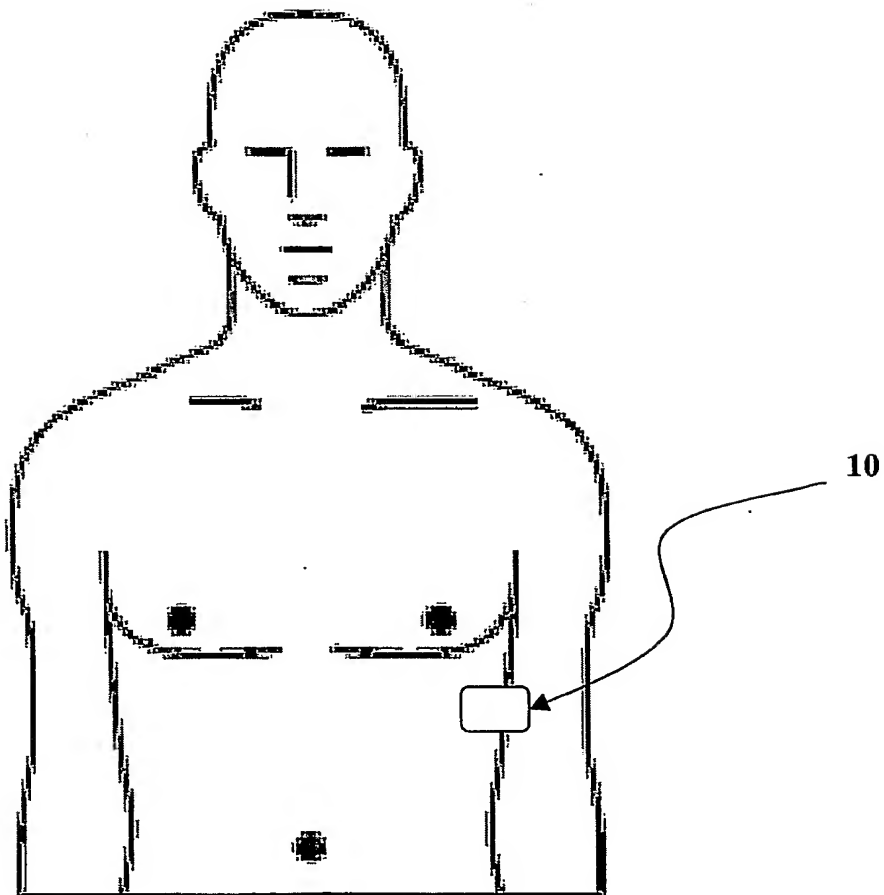

**FIG 2**


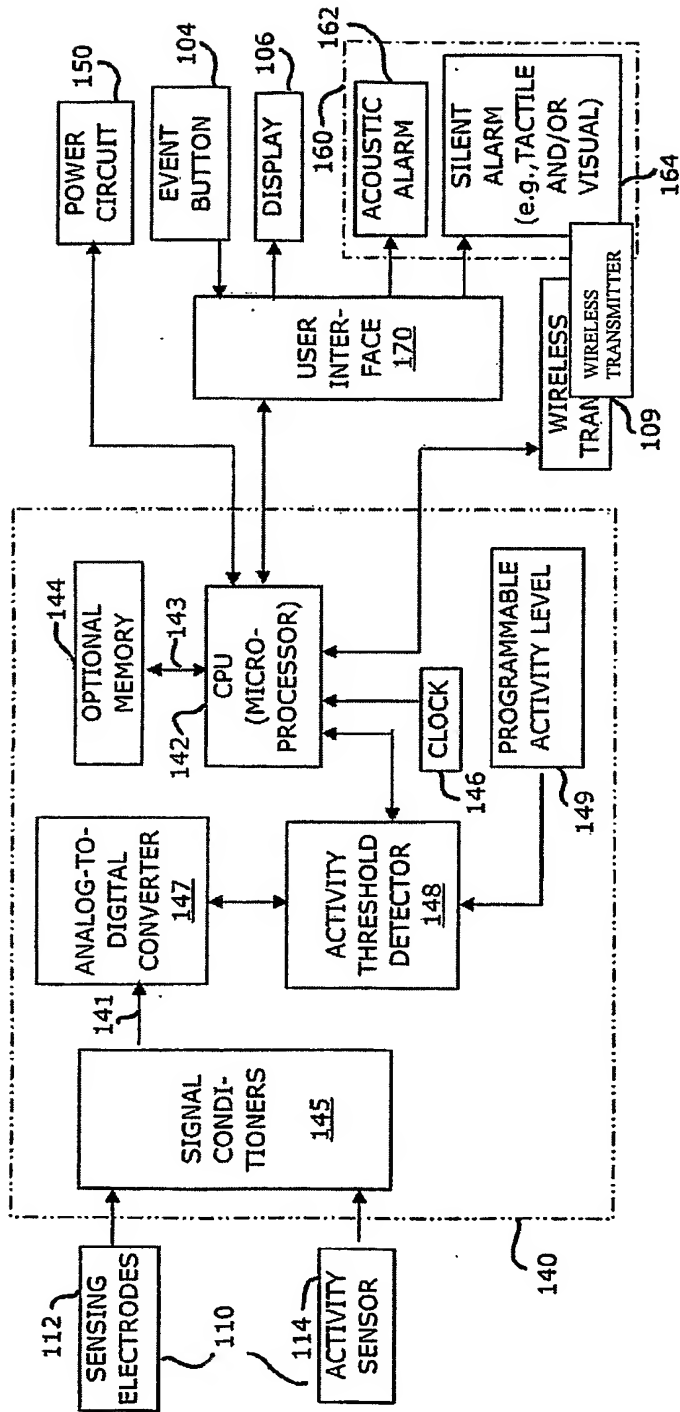


FIG 3



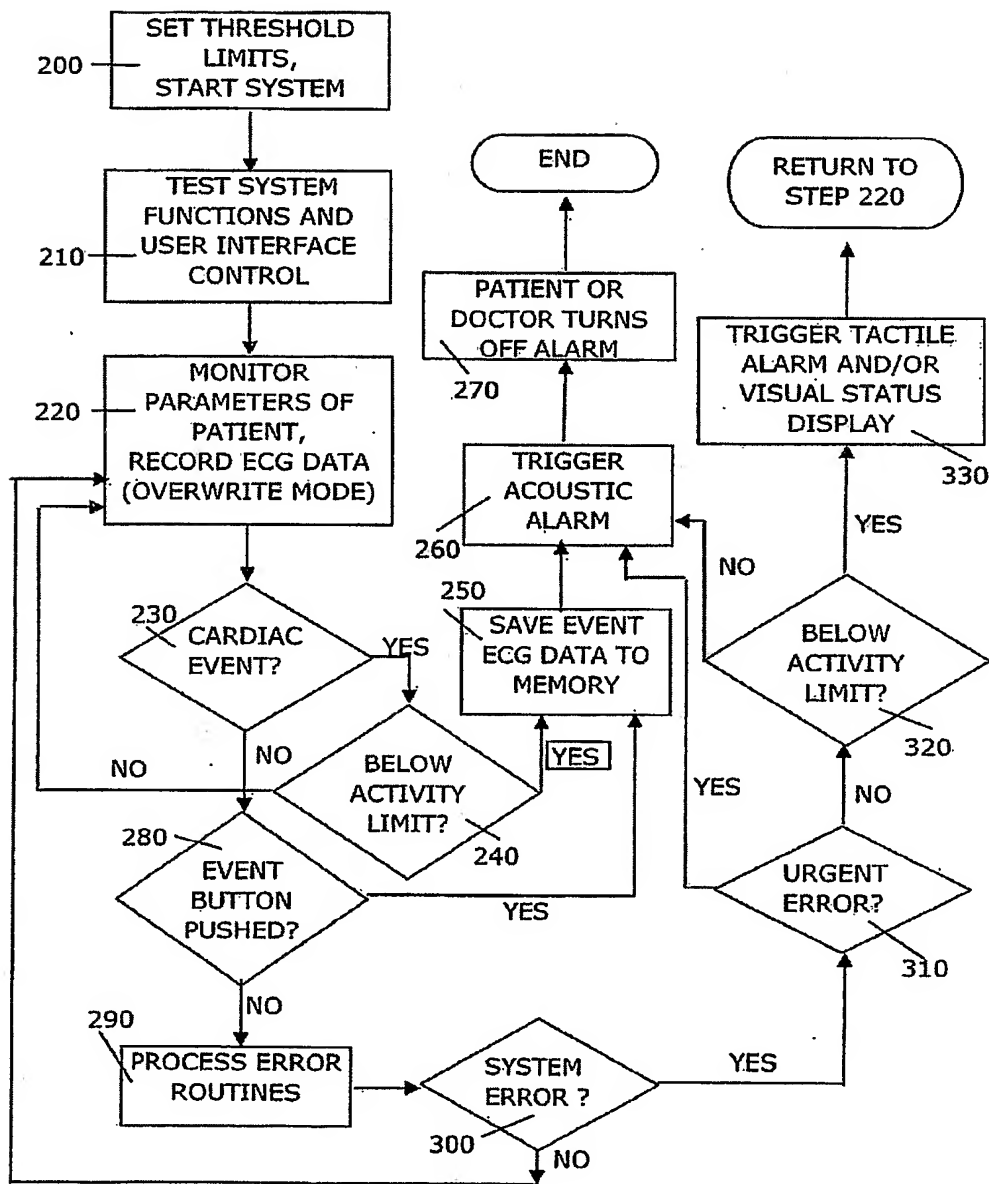

**FIG 4**